trister®
• Convenience • Confidence • Control

QUICK REFERENCE GUIDE

ADVANCED BLOOD PRESSURE MONITOR WITH ECG TS 320BPEC

Download iBP ECG Plus


Google play | Download on the App Store

Connect TS 320BPEC via Bluetooth on Smartphones and Tablets



Press here to turn on Bluetooth


TS 320BPEC

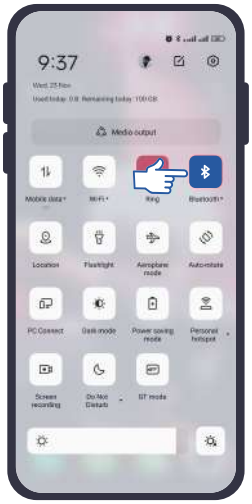


1.Turn on Mobile Bluetooth




2.Open iBP ECG Plus App

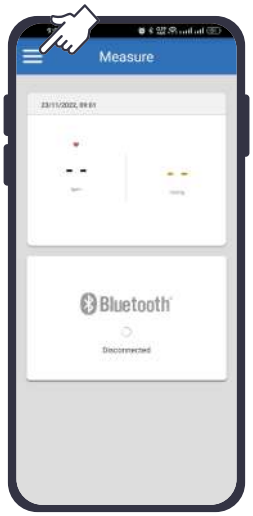


3.Touch the top three lines to open more options

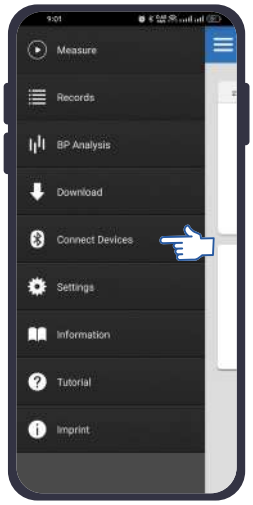

4. Go to Connect Devices

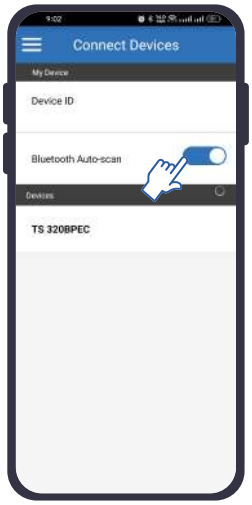

5. Turn on Auto-scan & Tap TS 320BPEC to establish connection.

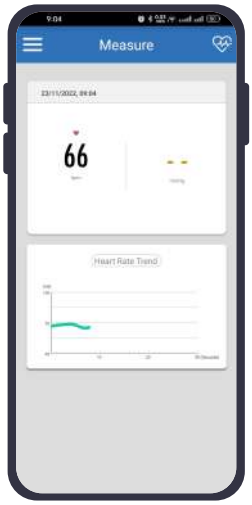

6. Start your measurement

Turn page to measurement Procedure




7. Result appear approximately 30 seconds.

Bluetooth Technology


With latest Bluetooth technology; Trister ECG BPM, provides real-time display of your ECG measurement on Smartphones/Tablets for reviewing your records and sharing with your healthcare provider.

Taking TS 320BPEC Measurement Procedure


- Connect the cable connector of ECG Pen to the port on the right side of the device.




- Lay your right index finger on the hollow part of top electrode and hold the ECG Pen in your right hand.

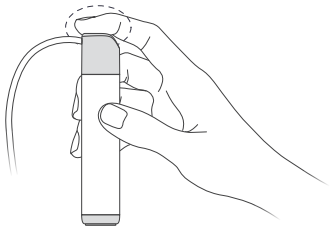


- Place the bottom electrodes on bare skin about 5 centimeters (2 inches) below your left nipple supported by the ribcage. Press the ECG Pen GENTLY until you hear the click sound.

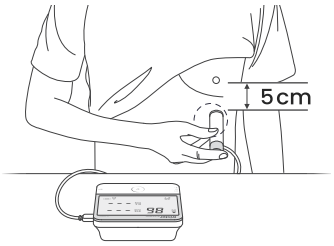

- **Note :** The force should be kept constant during the measuring period. Do not press the electrodes hard. Excessive muscle tension might affect the accuracy of measurement result.



- The Digits Display shows 30 seconds of count down and the ECG symbol will stay on after the ECG measurement start.

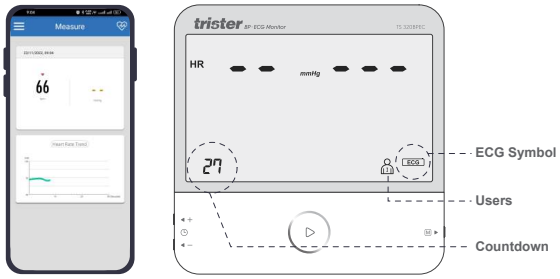

- During ECG measurement :
  - Measuring period will count down from 30 seconds.
  - The heart rate digits will dynamically show the real-time heartbeat.

- **Note:** The Averaged Heart Rate will only be displayed once the measurement is completed.

www.trister.com
info@trister.com

The Good Health Company